



Procedure of remove existed USB driver for DailyCare ECG recorder


Step1: Click "Control Panel"

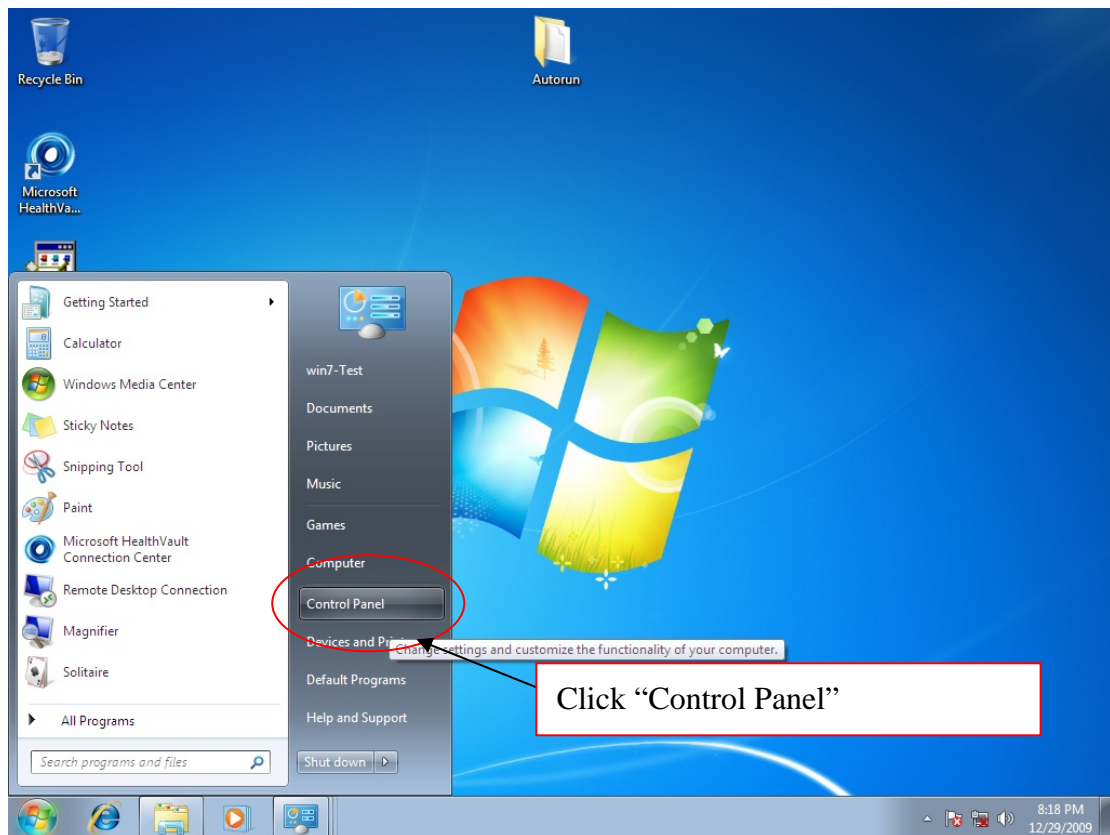


Step2: Click "Uninstall a program"

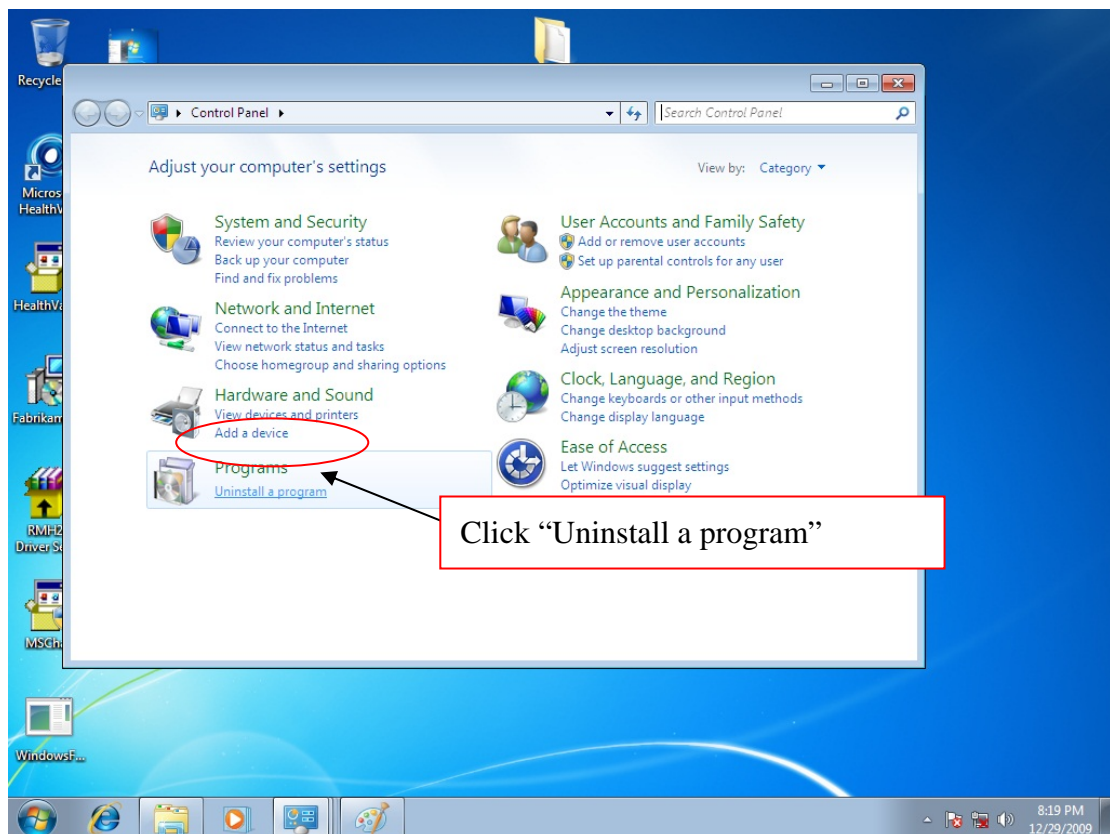


Step3: Select PL-2303 Driver

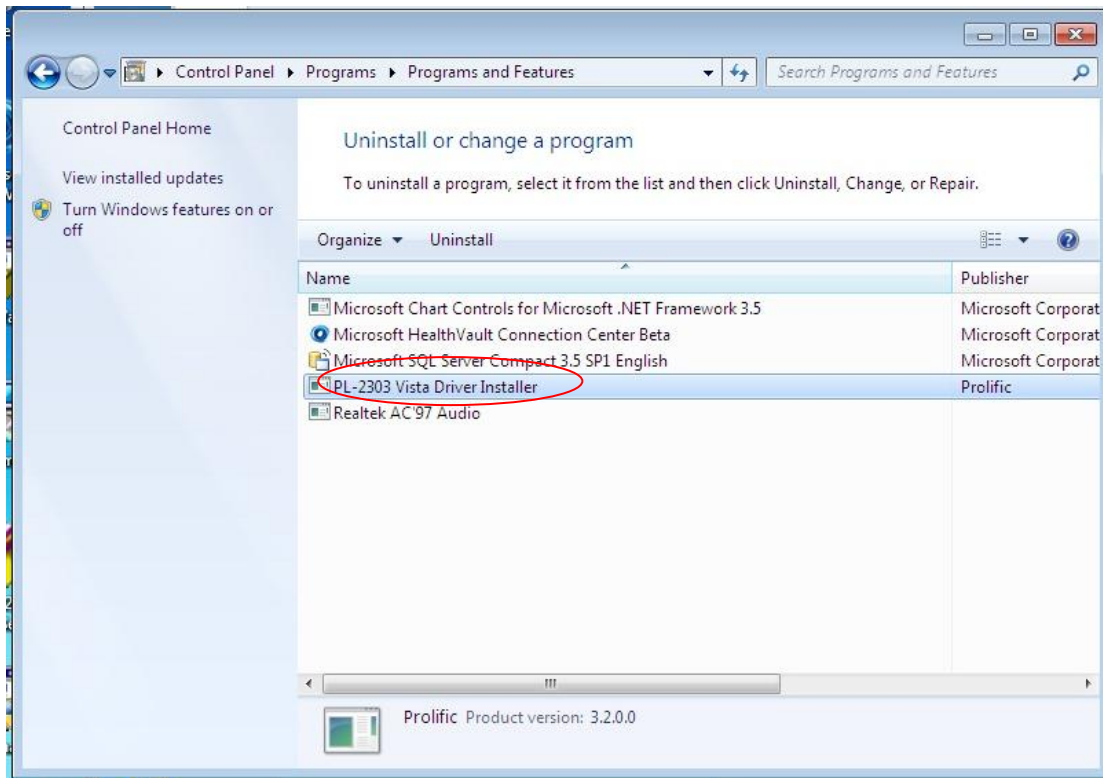

Step 4: Click "Uninstall"

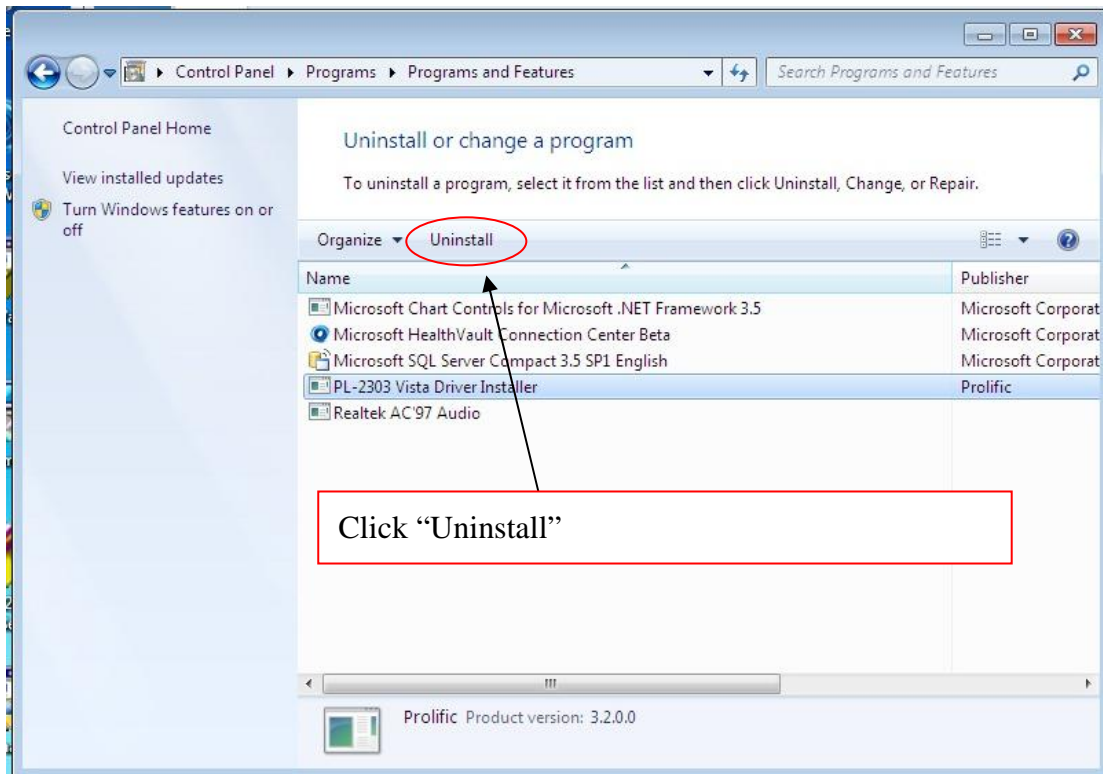

Step 5: Click Yes to uninstall USB driver

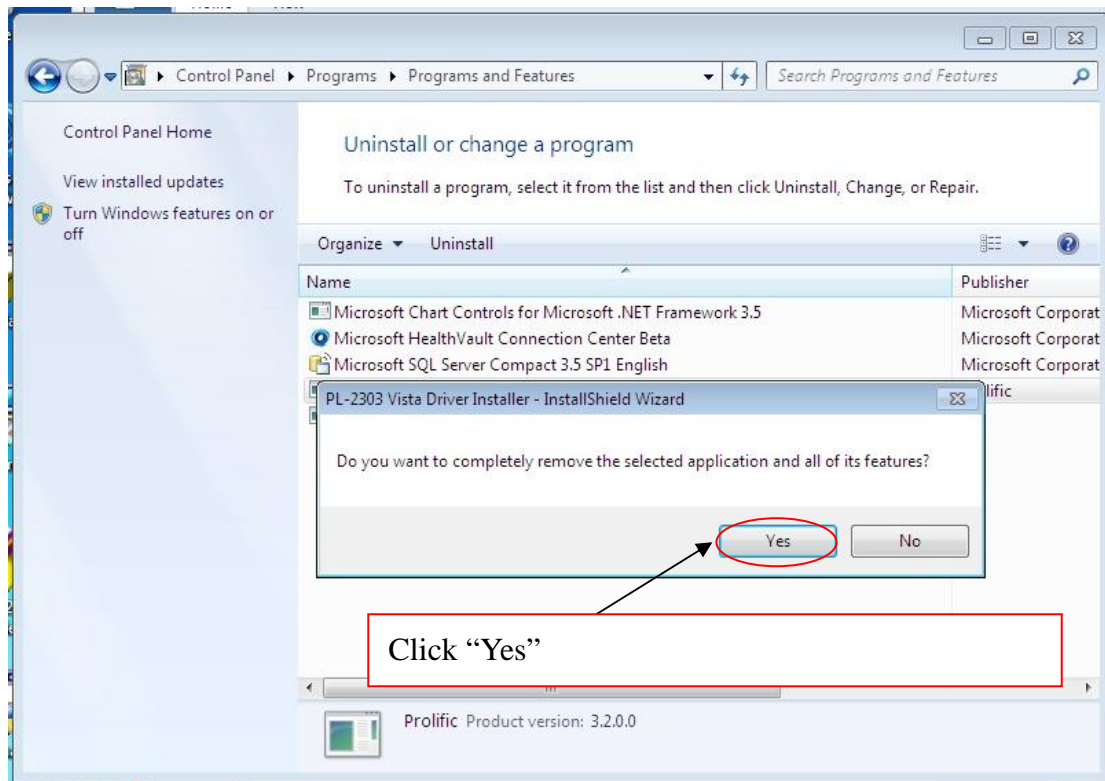

Step 6: Click "Finish".

